


## HEMODYNAMIC MONITORING: WHAT'S NEW?

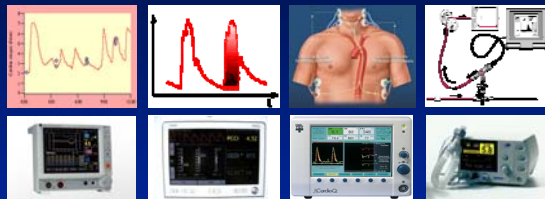

Michael L. Cheatham, MD, FACS, FCCM  
Director, Surgical Intensive Care Units  
Orlando Regional Medical Center

## OBJECTIVES

- To discuss the need for hemodynamic monitoring in the critically ill patient
- To review the various techniques currently available for assessing hemodynamic function in the ICU
- To describe the relative merits and limitations of the various monitoring techniques

## DISCLAIMERS

- I have no financial relationship with any company that produces hemodynamic monitoring equipment
- I will not be mentioning companies or products by name, but rather speaking about generic technologies
- Chances are that I will either not speak about your favorite technology or will have negative comments about it
- We are comparing technologies and their application in monitoring the sickest patients in our ICUs

## WHY DO WE MONITOR?

- Preload, contractility, afterload, and oxygen transport are commonly abnormal in the critically ill
- Inadequate resuscitation and failure to restore cellular oxygen delivery and organ perfusion results in multiple system organ failure (MSOF) and death
- Optimization of cardiopulmonary function during critical illness reduces organ failure and improves survival
- Accurate assessment of hemodynamic function and goal-directed resuscitation is essential to improving patient outcome

## CURRENT MONITORING TECHNOLOGIES

### Invasive Monitoring Techniques

- **Bolus thermodilution PAC**
- **Continuous thermodilution PAC**
- **Central venous oxygen saturation (ScvO<sub>2</sub>)**
- **Arterial Pulse Contour Analysis**

### Noninvasive Monitoring Techniques

- **Ultrasound**
- Thoracic Electrical Bioimpedance
- Partial Carbon Dioxide Rebreathing


## PULMONARY ARTERY CATHETER (PAC)

- Originally described by Swan & Ganz (1972)
- The “gold standard” for the next two decades
- Allows assessment of
  - Preload
    - Pulmonary artery occlusion pressure (PAOP)
    - Central venous pressure (CVP)
  - Contractility
    - Cardiac output (CO)
  - Afterload
    - Systemic vascular resistance (SVR)



### ARE WE MISSING TOO MUCH?


- Significant physiologic changes may go undetected by conventional intermittent monitoring techniques
  - A “snapshot” in time when a “moving picture” is what is needed

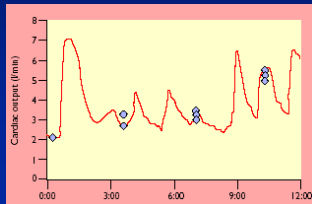


### CONTINUOUS THERMODILUTION

- Utilizes pulsed thermal energy technology
- Provides an updated hemodynamic assessment every 60 seconds
  - Automates CO measurement
  - Averages respiratory cycle variation
  - Standardizes injection technique
- Provides a constantly updated assessment of patient response to resuscitation leading to more efficient, goal-directed resuscitation

### INTERMITTENT THERMODILUTION

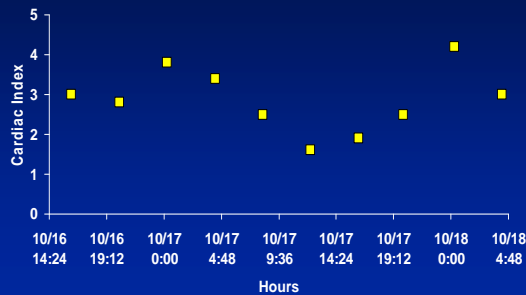

### CONTINUOUS THERMODILUTION

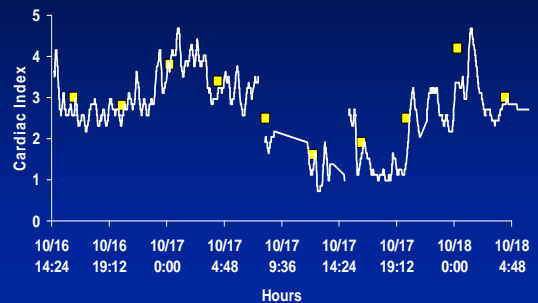

### LIMITATIONS OF CONTINUOUS THERMODILUTION

- Accuracy may be decreased by
  - Irregular heart rate and/or rhythm
  - Mitral valve disease
  - Incorrect catheter placement
  - Hyperthermia (> 41° Celsius)
- Data obtained must guide interventions to justify the risk – benefit ratio of the PAC
- The patient outcome benefits are achieved at the cost of increased data complexity and intensivist time

### CONTINUOUS THERMODILUTION

- Most invasive and labor-intensive of the monitoring technologies demanding a thorough understanding of PAC monitoring principles
- Provides a continuous assessment of
  - preload (RVEDV, PAOP, CVP)
  - contractility (CO)
  - afterload (SVR, RVEF)
  - oxygen transport balance (SvO<sub>2</sub>)
- Improves patient resuscitation and outcome
- Appropriate for the most critically ill patients



## CENTRAL VENOUS OXYGEN SATURATION

- Restoration of oxygen transport balance is essential
- Central venous oxygen saturation (ScvO<sub>2</sub>) monitoring allows continuous assessment of oxygen transport balance without a PAC
- ScvO<sub>2</sub> has gained widespread interest as a primary tool of EGDT and is advocated by the Surviving Sepsis Campaign



Rivers NEJM 2001

## LIMITATIONS OF CENTRAL VENOUS OXYGEN SATURATION



- Requires an invasive indwelling catheter
- Does not provide an accurate estimate of preload or a measurement of contractility
- SvO<sub>2</sub> and ScvO<sub>2</sub> are not equivalent
  - Trend in ScvO<sub>2</sub> over time, however, has significant clinical application and may represent one of the key features behind the success of EGDT

## CENTRAL VENOUS OXYGEN SATURATION

- Provides a continuous assessment of
  - preload (CVP)
  - oxygen transport balance (ScvO<sub>2</sub>)
- ScvO<sub>2</sub> is as simple as inserting a CVC, requires minimal interpretation, and may be initiated prior to ICU admission
  - Allows earlier assessment and resuscitation
- Expensive, but a useful early tool for identifying critical illness and beginning EGDT

## ARTERIAL PULSE CONTOUR ANALYSIS

- Estimation of stroke volume from the arterial pressure waveform was first described almost 100 years ago
  - CO is proportional to the area under the arterial pressure waveform
- Proposed as a less invasive alternative to the PAC
- Requires only an arterial pressure catheter and a central venous catheter (CVC)



## ARTERIAL PULSE CONTOUR ANALYSIS

- Three different technologies are currently available
  - Iced saline indicator calibration
  - Lithium indicator dilution calibration
  - Computer algorithm
- Two of these technologies require initial indicator dilution calibration
- All three technologies provide varying degrees of hemodynamic information

## COLD SALINE CALIBRATION TECHNIQUE

- An initial CO is determined using iced saline thermolodilution for calibration with subsequent measurements obtained using pulse contour analysis
- Provides continuous assessment of
  - Stroke volume (SV) and CO
  - Stroke volume variation (SVV)
    - Variation in beat-to-beat SV during a single respiratory cycle
- Provides intermittent assessment of
  - Global end-diastolic volume (GEDV)
  - Intrathoracic blood volume (ITBV)
  - Extravascular lung water (EVLW)

### LIMITATIONS OF COLD SALINE CALIBRATION TECHNIQUE


- Recalibration is necessary at least every 8 hours
- Not all measurements are continuous
- Accuracy is dependent upon
  - Arterial catheter location
    - Axillary / femoral more accurate than radial
  - Absence of aortic regurgitation, arrhythmias, intracardiac shunts, aortic aneurysms
  - Fully ventilated patient with stable heart rhythm

### COLD SALINE CALIBRATION TECHNIQUE

- A less invasive alternative to a PAC
- Provides continuous assessment of
  - Preload (SVV)
  - Contractility (CO)
- Provides intermittent assessment of
  - Preload (GEDV, ITBV, EVLW)
  - Contractility (CO)
  - Afterload (SVR) (requires CVC for CVP)
- Can answer the “volume or catecholamine” question
- A viable option for minimally invasive continuous hemodynamic monitoring


### LITHIUM INDICATOR DILUTION

- Utilizes pulse contour analysis via the patient's arterial catheter to measure CO, SV, and SVV
- Initial calibration is via indicator dilution using a lithium bolus and lithium-selective electrode



### LITHIUM INDICATOR DILUTION

- Accuracy is dependent upon arterial resistance, compliance, and impedance
  - Initial calibration via indicator dilution is required
  - Recalibration is necessary every 8 hours
- The bedside monitor contains a variety of monitoring screens and assessment tools

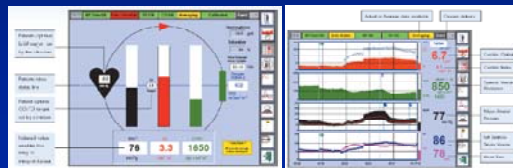

### LIMITATIONS OF LITHIUM INDICATOR DILUTION

- Cannot be used in patients on lithium therapy
- Lithium indicator is contraindicated in patients < 40 kg and during the first trimester of pregnancy
- Neuromuscular blocking agents can interfere with the lithium electrode
- Accuracy is dependent upon
  - Frequent recalibration
  - Arterial catheter location
  - Absence of aortic regurgitation, arrhythmias, intracardiac shunts, aortic aneurysms

### LITHIUM INDICATOR DILUTION

- Another less invasive alternative to a PAC
- Provides continuous assessment of
  - preload (SV, SVV)
  - contractility (CO)
  - afterload (SVR) (requires CVC for CVP)
- Bedside monitor is very user-friendly
- A viable option for minimally invasive continuous hemodynamic monitoring

### COMPUTER ALGORITHM

- Utilizes pulse contour analysis via the patient's arterial catheter to measure CO, SV, and SVV
- Can also measure SvO<sub>2</sub> or ScvO<sub>2</sub> if appropriate catheters are in place
- Does not require indicator dilution for initial calibration
  - Utilizes a computer algorithm based upon pulse pressure and a mathematical model for vascular tone based upon patient gender, height, weight, and BSA

### COMPUTER ALGORITHM

- Accuracy is dependent upon arterial resistance, compliance, and impedance
- Provides a continuously updated CO, SV, and SVV every 20 seconds
- Currently requires that the patient is mechanically ventilated and without significant arrhythmias




### COMPUTER ALGORITHM

- Another less invasive alternative to a PAC
- Provides continuous assessment of
  - preload (SV, SVV)
  - contractility (CO)
  - oxygen transport (SvO<sub>2</sub>, ScvO<sub>2</sub>)
- A viable option for minimally invasive continuous hemodynamic monitoring

### ULTRASOUND

- Several different methods exist for applying ultrasound to hemodynamic monitoring
  - 2-D echocardiography
    - Transthoracic
    - Transesophageal (TEE)
  - Esophageal Doppler
  - Transcutaneous ultrasound



### 2-D ECHOCARDIOGRAPHY


- Provides information of cardiac structure and mechanical function
- Useful for assessing valvular anatomy and function as well as for aortic injury
- Can identify the presence of pericardial fluid
- Useful for assessing preload and contractility

### LIMITATIONS OF 2-D ECHOCARDIOGRAPHY

- Both
  - Not a continuous monitoring technology
- Transthoracic (TTE)
  - 10-40% failure rate in ICU due to patient anatomy
- Transesophageal (TEE)
  - Requires a sedated patient; may require neuromuscular blockade
  - Contraindicated in patients with esophageal disease or difficult airway

## 2-D ECHOCARDIOGRAPHY

- An alternative to a PAC
  - Arguably invasive
- Provides information not available with other techniques
- Provides assessment of
  - preload (LVEDV, LVEDA)
  - contractility (CO, LVEF)
  - valve function
  - pericardial fluid
- An essential technology for intermittently assessing the critically ill patient



## ESOPHAGEAL DOPPLER

- First described as a method for measuring CO in 1971
- Based upon measurement of blood flow velocity in the descending aorta
  - Requires either measurement or estimation of cross-sectional aortic diameter



## ESOPHAGEAL DOPPLER

- Provides “continuous” assessment of
  - SV and CO
  - Corrected flow time (FTc)
    - A preload estimate superior to PAOP and CVP in predicting preload recruitable increases in CO
  - Peak flow velocity
    - An estimate of ventricular contractility
  - Total SVR
    - Estimated SVR based on aortic blood flow
- Generally feasible only for short-term, intermittent monitoring

## LIMITATIONS OF ESOPHAGEAL DOPPLER

- Proper positioning of the Doppler probe is essential
- There is a learning curve
  - Operator technique and experience directly impact upon measurement accuracy
- Requires a sedated or intubated patient
- May not be appropriate for patients with
  - Severe agitation
  - Bleeding diatheses
  - Esophageal varices
  - Aortic dissection

## ESOPHAGEAL DOPPLER

- An alternative to a PAC
  - Arguably invasive
- Provides continuous assessment of
  - preload (SV, FTc)
  - contractility (CO, peak flow velocity)
  - afterload (estimated) (TSVR)
- A viable option for intermittent hemodynamic assessment or screening patients for hemodynamic abnormalities

## TRANSCUTANEOUS ULTRASOUND

- Utilizes continuous wave Doppler ultrasound coupled with specialized algorithms and signal processing to non-invasively assess hemodynamic function
- A portable monitor allows measurements in a variety of clinical settings



### TRANSCUTANEOUS ULTRASOUND

- Provides “continuous” assessment of
  - SV
  - CO
  - SVV
  - Corrected flow time (FTc)
  - Peak flow velocity
  - SVR
- Feasible for short-term, intermittent monitoring

### LIMITATIONS OF ULTRASOUND

- Proper positioning of the transducer is essential
- There is a learning curve
  - Operator technique and experience directly impact upon measurement accuracy
- Accuracy may be limited in the presence of:
  - Subcutaneous air or bone
  - Obesity
  - Valvular abnormalities
  - Significant respiratory disease

### TRANSCUTANEOUS ULTRASOUND

- A noninvasive alternative to a PAC
- Provides continuous assessment of
  - preload (SV, SVV, FTc)
  - contractility (CO, peak flow velocity)
  - afterload (SVR) (requires CVC)
- A viable option for intermittent hemodynamic assessment or screening patients for hemodynamic abnormalities

### TECHNOLOGY COMPARISON:

| Technology          | Preload          | Contractility | Afterload | O <sub>2</sub> Trans | Cost   |
|---------------------|------------------|---------------|-----------|----------------------|--------|
| Continuous TD       | PAOP, CVP, RVEDV | CO, RVEF      | SVR       | SvO <sub>2</sub>     | \$\$\$ |
| Bolus TD            | PAOP, CVP        | CO            | SVR       |                      | \$     |
| ScvO <sub>2</sub>   |                  |               |           | ScvO <sub>2</sub>    | \$\$   |
| Cold Saline         | GEDV, SVV        | CO            | SVR       |                      | \$\$   |
| Lithium Dilution    | SVV              | CO            | SVR       |                      | \$\$\$ |
| Computer Alg        | SVV              | CO            | SVR       | ScvO <sub>2</sub>    | \$\$   |
| TTE / TEE           | LVEDV            | CO            |           |                      | \$     |
| Esoph Doppler       | FTc              | CO            |           |                      | \$     |
| Transcut Ultrasound | FTc, SVV         | CO            | SVR       |                      | \$\$   |
| Bioimpedance        | SV               | CO            | SVR       |                      | \$\$\$ |
| Partial Rebreathing |                  | CO            |           |                      | \$\$   |

↑ INVASIVENESS

### CONCLUSIONS

- The currently available monitoring technologies vary in the cost and diversity of information provided
- The more invasive techniques generally provide the most accurate and comprehensive data
- Critically ill patients may benefit from the more invasive techniques as a result of the greater breadth of information gained
- Physicians must thoroughly understand the hemodynamic data obtained and utilize it in a goal-directed fashion if the monitoring technology is to improve patient outcome